


Cardinal Health™ PRO/PRO to GO  
Negative Pressure Wound Therapy

Clinician Quick Reference Guide



**NOTE:** Please refer to the Cardinal Health™ Negative Pressure Wound Therapy (NPWT) PRO/PRO to GO Clinician User Manual for detailed instructions and review the Precautions and Contraindications before use.

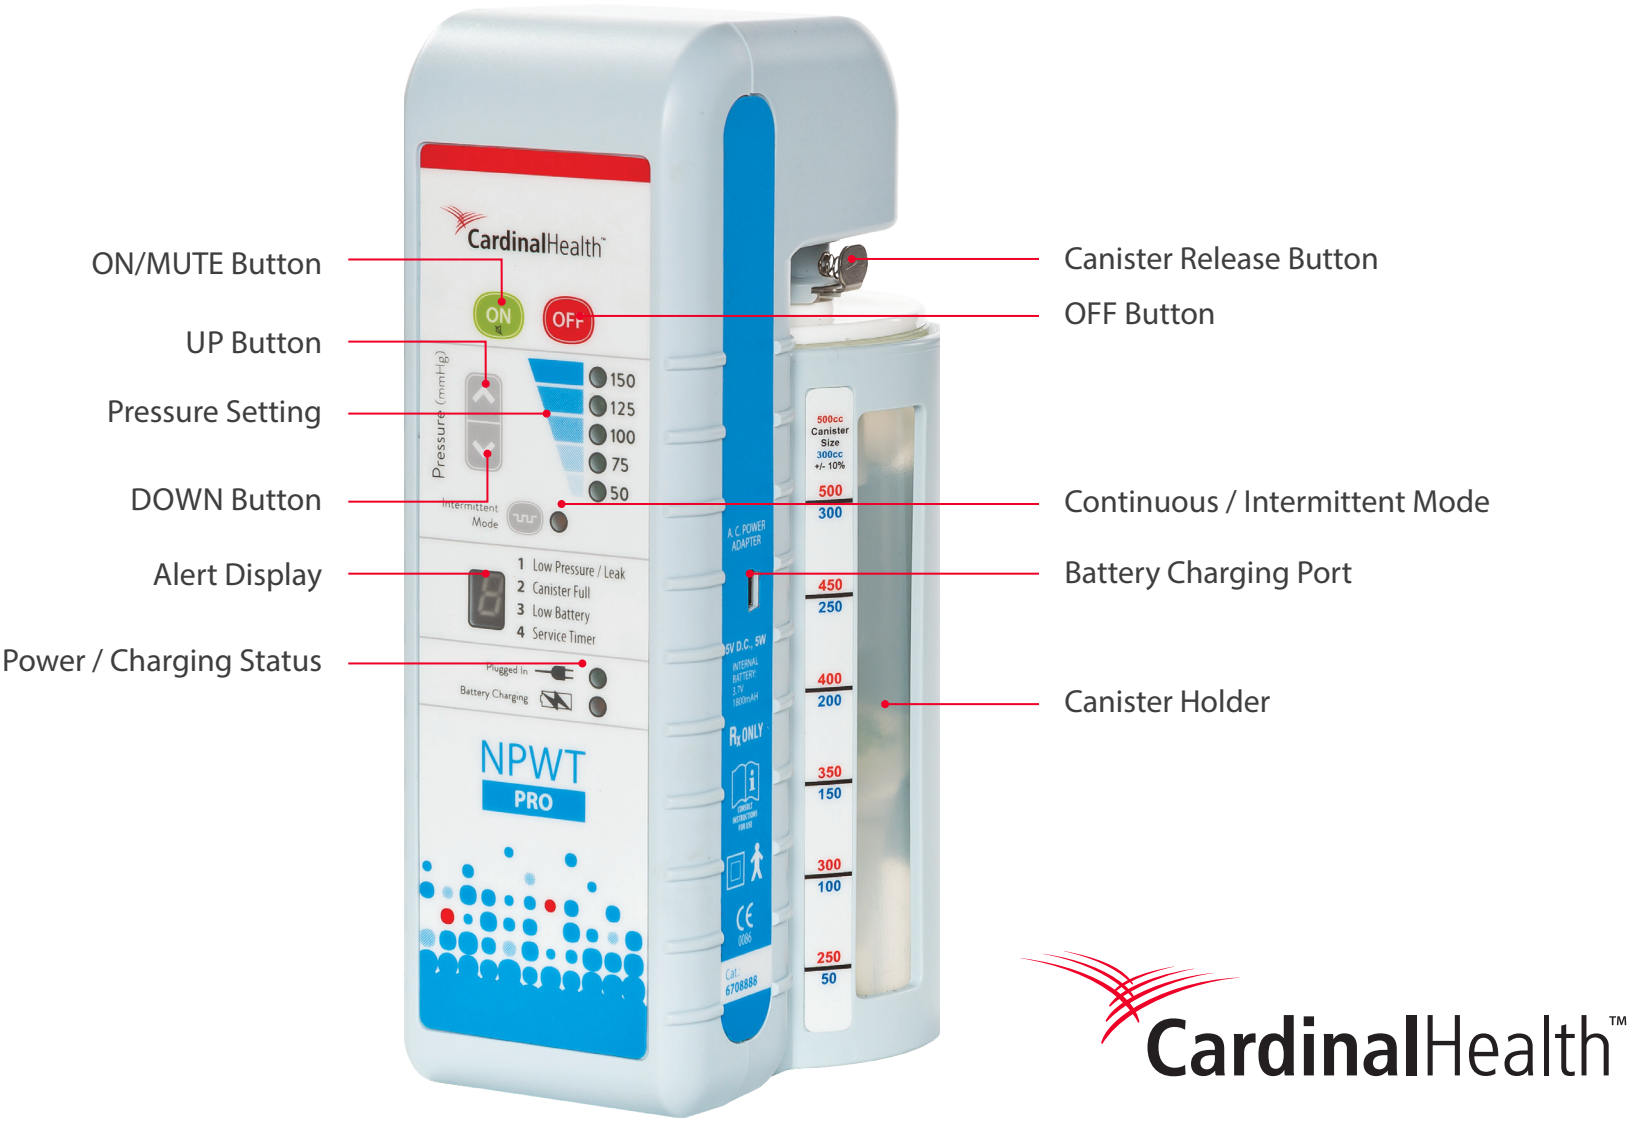


Insert Canister

Insert canister in holder by sliding it up into bottom of the Canister Holder. Line up the two short ports with the Canister Holder and press until it “clicks” into place and locks. To remove canister, press Canister Release Button, grasp canister at bottom and pull downward.


Connect the Dressing

Connect the blue end of the tubing to the open port of the canister. Gently twist and push connector on just enough to seal it. Make sure that the clamp on the tubing is open.  
**NOTE:** Please refer to the Cardinal Health™ NPWT PRO/PRO to GO Clinician User Manual for instructions on how to properly dress the wound and troubleshoot issues.


Turning the PRO/PRO to GO ON

Press the ON  button to start therapy. Select the desired Pressure Setting by pressing the UP  or DOWN  arrow button. A green light begins flashing next to the selected Pressure Setting. The light flashes and remains lit when the set pressure is reached. The light flashes if the pressure cannot be maintained.




Therapy Lockout

To lock Therapy Setting, press and hold the ON  button for 3 seconds. The PRO/PRO to GO beeps three times indicating negative pressure wound Therapy Setting is locked. Repeat process to unlock negative pressure wound Therapy Setting.

Intermittent Mode

To operate the device in Intermittent Mode, press the Intermittent Mode  Button. An amber light indicates the PRO/PRO to GO is operating in Intermittent Mode. Repeat process to return to Continuous Mode.

Adjust Alert Volume

Volume may be adjusted by pressing and holding the ON  Button and tapping the UP  or DOWN  arrow button. The numbers 1 to 5 will appear in the Alert Display. The No. 1 is the lowest; No. 5 is the highest volume level.

Troubleshooting

If the PRO/PRO to GO begins to alert, refer to the troubleshooting table on the back.

Turning the PRO/PRO to GO OFF

To turn PRO/PRO to GO off, press the OFF  Button. The Alert Display flashes “o-f-f” three times while the PRO/PRO to GO is preparing to shut down.



For questions or information, contact Cardinal Health at 1.866.484.6798

**Notice to Users:** As with any prescription medical device, failure to follow product instructions or adjusting settings and performing therapy applications without the express direction and/or supervision of your trained clinical caregiver may lead to improper product performance and the potential for serious or fatal injury.

**Defibrillation:** Remove the wound dressing if defibrillation is required in the area of dressing placement. Failure to remove the dressing may inhibit electrical current transmission and/or patient resuscitation.

**Magnetic Resonance Imaging (MRI):** The PRO/PRO to GO is not MRI-compatible. Do not take into the MRI area.

**Hyperbaric Oxygen Therapy (HBO):** NEVER allow a device — whether on or off — inside a hyperbaric chamber. The PRO/PRO to GO must be disconnected from the patient prior to HBO treatment.

What you see or hear	Problem	What to do	More Information
<b>Low Pressure/Leak</b> <b>“1” flashing in Alert Display.</b> <b>Single beep.</b> <b>PRO/PRO to GO is making more noise.</b>	<p>There is an air leak in either the dressing or the tubing connections.</p> <p>Leaks often occur over areas of moist skin, creases or folds in skin and wrinkles in the drape. They can occur if the drape snags on clothing or bedsheets.</p>	<ul style="list-style-type: none"> <li>•Clamp the tubing.</li> <li>•Look for leaks in the dressing. Gently press around the dressing to check for leaks. If leak is found, use the extra drape or drape strips to seal.</li> <li>•If the alert continues, check the tubing connection to the canister and make sure the tubing is secure by twisting the connector clockwise.</li> <li>•If alert continues, make sure the canister is fully seated and locked in the PRO/PRO to GO. Check for cracks in the canister. If found, replace the canister.</li> <li>•If alert continues, check the tubing for leaks. If a leak is found in the tubing, the entire dressing and tubing set must be replaced.</li> <li>•Open the clamp.</li> </ul>	<p>If the leak is properly sealed, the pump becomes quiet and the alert stops. If alert continues, call Cardinal Health at 1.866.484.6798.</p>
<b>Canister Full</b> <b>“2” flashing in Alert Display.</b> <b>Two beeps.</b>	<p>The canister is full.</p>	<ul style="list-style-type: none"> <li>•Make sure clamp is open.</li> <li>•Visually assess the canister to see if full. If the canister is full, change the canister.</li> <li>•If the canister is not full, turn the PRO/PRO to GO off by pressing the OFF  button and then turn the PRO/PRO to GO back on to resume therapy.</li> </ul>	<p>The Canister Full alert begins when the canister is 90 percent full, but the PRO/PRO to GO will continue to work until the canister completely fills.</p> <p>If the PRO/PRO to GO is placed on its front, fluid entering the canister will cause a false Canister Full alert and the canister must be changed.</p> <p>If alert continues, call Cardinal Health at 1.866.484.6798 for more assistance.</p>
<b>Low Battery</b> <b>“3” flashing in Alert Display.</b> <b>Three beeps.</b>	<p>The battery is low and has approximately 30 minutes before the battery will be too low to support continued operation of the PRO/PRO to GO.</p>	<p>Plug in the PRO/PRO to GO. A green light shows next to the Plugged In symbol and a yellow light shows next to the Battery Charging symbol to indicate that the battery is charging. The yellow light turns off after the battery is fully charged.</p>	<p>Use only the A.C. Power Adapter that came with the PRO/PRO to GO.</p> <p>If alert continues or replacement A.C. Power Adapter is needed, call Cardinal Health at 1.866.484.6798 for assistance.</p>
<b>Service Needed</b> <b>“4” flashing in Alert Display.</b> <b>Four beeps.</b>	<p>PRO/PRO to Go needs to be serviced.</p>	<p>Call Cardinal Health at 1.866.484.6798 for assistance.</p>	<p>This alert cannot be muted or manually reset by turning the PRO/PRO to GO off and on.</p>
<b>Pressure Setting will not change.</b>	<p>Pressure lock-out is engaged.</p>	<ul style="list-style-type: none"> <li>•Unlock the PRO/PRO to GO by pressing and holding ON button for 3 seconds.</li> <li>•The PRO/PRO to GO beeps three times indicating that the setting is unlocked.</li> </ul>	<p>To lock therapy setting, press and hold the ON  button for 3 seconds. The PRO/PRO to GO beeps three times indicating Pressure Setting is locked.</p>
<b>PRO/PRO to GO is quiet and fluid is not moving in the tubing.</b>	<p>This is NOT a problem.</p>	<p>No action needed.</p>	<p>Change the PRO/PRO to GO to Intermittent Mode to move fluid from the tubing into the canister.</p>
<b>An amber light is showing on the front of the PRO/PRO to GO below the pressure numbers.</b>	<p>This is NOT a problem. The PRO/PRO to GO is operating in Intermittent Mode.</p>	<p>No action needed.</p>	<p>Intermittent Mode maintains target pressure for 5 minutes and decreases to -25mmHg for 2 minutes.</p>