

Allegra 21 Series, GS-15 Series, and Spinchron 15 Series Centrifuges

Instruction Manual



Symbol Simbolo Symbol 記号 Symbole 符号 Símbolo	Title / Titel / Titre / Titulo / Titolo / 名称 / 名称
4	Dangerous voltage Gefährliche elektrische Spannung Courant haute tension Voltaje peligroso Pericolo: alta tensione 危険電圧 危险电压
<u></u>	Attention, consult accompanying documents Achtung! Begleitpapiere beachten! Attention, consulter les documents joints Atención, consulte los documentos adjuntos Attenzione: consultare le informazioni allegate 注意、添付資料を参照のこと 注意,请参阅附帯的文件
	On (power) Ein (Netzverbindung) Marche (mise sous tension) Encendido Acceso (sotto tensione) 入(電源) 开(电源)
	Off (power) Aus (Netzverbindung) Arrêt (mise hors tension) Apagado Spento (fuori tensione) 切(電源) 关 (电源)
	Protective earth (ground) Schutzleiteranschluß Liaison à la terre Puesta a tierra de protección Collegamento di protezione a terra 保護アース(接地)
<u></u>	Earth (ground) Erde Terre Tierra Scarica a terra アース(接地)



This safety notice summarizes information basic to the safe operation of the equipment described in this manual. The international symbol displayed above is a reminder that all safety instructions should be read and understood before installation, operation, maintenance, or repair of this instrument. When you see the symbol on other pages, pay special attention to the safety information presented. Observance of safety precautions will also help to avoid actions that could damage or adversely affect the performance of the instrument.

Other symbols may also be displayed on the equipment. These are reproduced and described on the reverse side of the cover page.

Safety During Installation and/or Maintenance

These centrifuges each weigh 50 kg/110.3 lb (nonrefrigerated model) or 70 kg/154.4 lb (refrigerated model). DO NOT attempt to lift or move one of them without assistance from another person.

Be sure to use the anchoring system to secure the centrifuge in place. The anchoring system is designed to reduce the possibility of injury or damage which could result from instrument movement in the event of a major rotor mishap.

Any servicing of this equipment that requires removal of any covers can expose parts which involve the risk of electric shock or personal injury. Make sure that the power switch is turned off and the instrument is disconnected from the main power source, and refer such servicing to qualified personnel.

Do not replace any centrifuge components with parts not specified for use on this instrument.

Electrical Safety

To reduce the risk of electrical shock, this equipment uses a three-wire electrical cord and plug to connect this equipment to earth-ground. To preserve this safety feature:

- Make sure that the matching wall outlet receptacle is properly wired and earth-grounded.
 Check that the line voltage agrees with the voltage listed on the name-rating plate affixed to the instrument.
- Never use a three-to-two wire plug adapter.
- Never use a two-wire extension cord or a two-wire non-grounding type of multiple-outlet receptacle strip.

Do not place containers holding liquid on or near the chamber door. If they spill, liquid may get into the instrument and damage electrical or mechanical components.

Safety Against Risk of Fire

Certain electrical circuits within this equipment are protected by fuses against overcurrent conditions. For continued protection against the risk of fire, replace only with the same type and rating specified.

This centrifuge is not designed for use with materials capable of developing flammable or explosive vapors. Do not centrifuge such materials (chloroform or ethyl alcohol for example)

in this instrument nor handle or store them within the 30-cm (1-ft) clearance envelope surrounding the centrifuge.

Mechanical Safety

For safe operation of the equipment, observe the following:

- Use only the Beckman Coulter rotors and accessories designed for use in this centrifuge.
- Before starting the centrifuge, make sure that the rotor tie-down screw is securely fastened.
- Do not exceed the maximum rated speed of the rotor in use.
- NEVER attempt to slow or stop the rotor by hand.
- Do not lift or move the centrifuge while the rotor is turning.
- If a glass tube breaks inside the chamber bowl, be careful when examining or cleaning the gasket or chamber, as sharp glass fragments may be embedded in their surfaces.
- NEVER attempt to override the door interlock system while the rotor is spinning.
- Maintain a 7.6-cm (3-in.) clearance envelope around the centrifuge (secured with antirotation kit) while it is running. During operation you should come within the envelope only to adjust instrument controls, if necessary. Never bring any flammable substances within the 30-cm (1-ft) area surrounding the centrifuge. Never lean on the centrifuge or place items on the centrifuge while it is operating.

Chemical and Biological Safety


Normal operation may involve the use of solutions and test samples that are pathogenic, toxic, or radioactive. Such materials should not be used in this instrument, however, unless all necessary safety precautions are taken.

- Observe all cautionary information printed on the original solution containers prior to their use.
- Because spills may generate aerosols, observe proper safety precautions for aerosol containment.
- Handle all infectious samples according to good laboratory practices and methods to prevent the spread of disease. Ask your laboratory safety officer to advise you about the level of containment required for your application and about the proper decontamination or sterilization procedures to follow if fluids escape from containers. Biosafe containment should be used when Risk Group II materials (as identified in the World Health Organization *Laboratory Biosafety Manual*) are handled; materials of a higher group require more than one level of protection. Because spills may generate aerosols, observe proper safety precautions for aerosol containment.
- Other infectious samples must also be handled according to good laboratory procedures and methods to prevent spread of disease.
- Dispose of all waste solutions according to appropriate environmental health and safety guidelines.

It is your responsibility to decontaminate the instrument and accessories before requesting service by our Field Service representative.

Allegra 21 Series, GS-15 Series, and Spinchron 15 Series Centrifuges

Instruction Manual

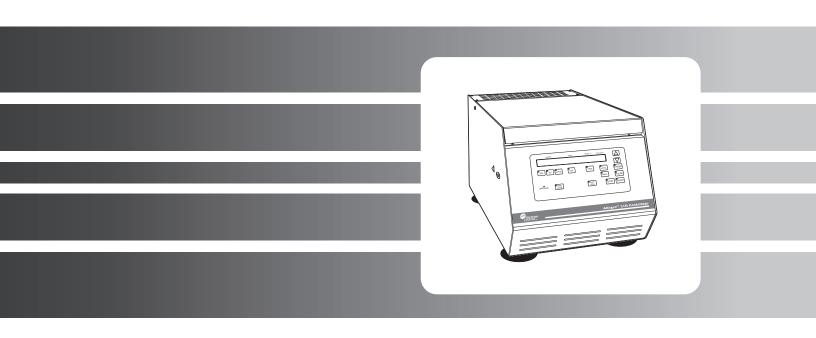

Contents

	Page
INTRODUCTION	ON
	CertificationviScope of ManualviConventionsviiCFC-Free CentrifugationxRadio Interferencex
	Recycling Label
	Nonrefrigerated Model Specifications
SECTION 1:	DESCRIPTION
	Instrument Function and Safety Features 1-1 Instrument Function 1-1 Models 1-2 Safety Features 1-3 Name Rating Plate 1-3 Chassis 1-4 Housing 1-4 Door 1-4 Rotor Chamber 1-4 Drive 1-5 Temperature Sensing and Control 1-5 Controls and Indicators 1-5 Power Switch 1-6 Control Panel 1-6
SECTION 2:	INSTALLATION
	Installing the Instrument. 2-1 Electrical Requirements 2-2 Test Run 2-4

	OPERATION	
	Run Procedure	5-2
	Preparation and Loading	-2
	Entering Run Parameters	3-5
	Starting a Run	10
	Changing Parameters During a Run	11
	Stopping a Run	12
	Unloading	12
	Summary of Run Procedures	13
SECTION 4:	TROUBLESHOOTING	
	User Messages	L -1
	Other Possible Problems	
	Emergency Access	
SECTION 5:	CARE AND MAINTENANCE	
2201101(0)	Maintenance	: າ
	Preventive Maintenance. 5	
	Replacing the Rotor Chamber Gasket	
	Cleaning	
	Tube Breakage	
	Decontamination	
	Sterilization and Disinfection	
	Storage and Transport	
	Storage and Transport	
	Storage and Transport	5-4
	Storage 5	5-4 5-4
	Storage	5-4 5-4 5-5

Page

Illustrations

	Page	•
Figure 1-1.	The Allegra 21 and Allegra 21R Centrifuges	2
Figure 1-2.	Interior View of the Rotor Chamber	1
Figure 1-3.	The Power Switch1-6	5
Figure 1-4.	The Control Panels	5
Figure 2-1.	Dimensions of the Nonrefrigerated and Refrigerated Centrifuges	3
Figure 3-1.	Tapered Sleeve Position	3
Figure 3-2.	Installing a Rotor	1
Figure 3-3.	Default Parameters	5
Figure 4-1.	Emergency Door Release	5
Figure 5-1.	Replacing the Rotor Chamber Gasket	2

Tables

		Page
Table 3-1.	Acceleration/Deceleration Times (in minutes:seconds)	3-9
Table 4-1.	Error Message Chart	4-2
Table 4-2	Troubleshooting Chart	4-4

CERTIFICATION

To ensure full system quality, Beckman Coulter Allegra 21 series, GS-15 series, and Spinchron 15 series centrifuges are manufactured in a registered ISO 9001 or 13485 facility. They have been designed and tested to be compliant (when used with Beckman rotors) with the laboratory equipment requirements of applicable regulatory agencies. Declarations of conformity and certificates of compliance are available at www.beckmancoulter.com.

International symbols that may be displayed on the centrifuge are illustrated and described on the reverse side of the cover page.

SCOPE OF MANUAL

This manual is designed to familiarize you with the Beckman Coulter Allegra 21 series, GS-15 series, and Spinchron 15 series benchtop centrifuges, their functions, specifications, operation, and routine operator care and maintenance.

- The following introductory pages contain the instrument specifications, as well as space, electrical, and temperature conditions required for optimal centrifuge performance. A list of available rotors is also included
- Section 1 provides a brief physical and functional description of the centrifuge and the operating controls and indicators.
- Section 2 contains instructions for installing and connecting the centrifuge.
- Procedures for operating the centrifuge are summarized in Section 3.

- Section 4 lists possible error messages and/or malfunctions, together with probable causes and corrective actions required.
- Procedures for operator care and maintenance are presented in Section 5, as well as a brief list of supplies and replacement parts.
- A Program Library chart is provided at the back of this manual. You can use this chart to record the parameters of a run for later duplication of the run conditions.

We recommend that you read this entire manual, especially the SAFETY NOTICE and all safety-related information, before operating the centrifuge or performing instrument maintenance.



If the centrifuge is used in a manner other than specified in this manual, the safety and performance of this equipment could be impaired. Further, the use of any equipment other than that intended for use by Beckman Coulter has not been evaluated for safety. Use of any equipment not specifically recommended in this manual is the sole responsibility of the user.

CONVENTIONS

NOTES, CAUTIONS, AND WARNINGS

Certain symbols are used in the manual to call out safety related and other important information. These are reproduced and described below and/or on the inside of the front cover.



Used to call attention to information that should be followed during installation, use, and/or servicing of the equipment.



CAUTION

Used to indicate a potential hazardous situation which, if not avoided, may result in minor or moderate injury and/or mechanical damage. It is also used to alert against unsafe practices.



WARNING

Used whenever an action or condition may potentially cause serious personal injury or loss of life. Mechanical damage may also result.



or

WARNING

Indicates high voltage or risk of electric shock. Turn the power switch off and disconnect the equipment from the main power source. Refer servicing of all areas displaying either symbol to a service personnel.

TYPOGRAPHIC CONVENTIONS

Certain typographic conventions are used throughout this manual to distinguish names of user interface components, such as keys and displays.

- Key names (for example, [START] or [ENTER]) appear in brackets.
- *Display names* (for example, **TEMP°C** or **SPEED**) appear in bold type.
- *Cursor keys*, used to increment values up or down when setting parameters, are shown as up and down arrows (▲ or ▼).

CFC-FREE CENTRIFUGATION



To ensure minimal environmental impact, no CFCs are used in the manufacture or operation of Allegra 21, GS-15, or Spinchron 15 series centrifuges.

RADIO INTERFERENCE

This instrument has been tested and found to comply with the limits for a Class A digital device, pursuant to Part 15 of FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with this instruction manual, may cause interference to radio communications. Operation of this equipment in a residential area may cause interference, in which case the user will be required to correct the interference at his or her own expense.

CANADIAN REGULATIONS

This digital apparatus does not exceed the Class A limits for radio noise emissions from digital apparatus as set out in the radio interference regulations of the Canadian Department of Communications.

Le présent appareil numérique n'émet pas de bruits radioélectriques dépassant les limites applicables aux appareils numériques de Classe A prescrites dans le reglement sur le brouillage radioelectrique édicté par le Ministère des Communications du Canada.

RECYCLING LABEL



Note: On the instrument, the triangle background is yellow rather than gray.

This symbol is required in accordance with the Waste Electrical and Electronic Equipment (WEEE) Directive of the European Union. The presence of this marking on the product indicates:

- 1) the device was put on the European market after August 13, 2005 and
- 2) the device is not to be disposed via the municipal waste collection system of any member state of the European Union.

It is very important that customers understand and follow all laws regarding the proper decontamination and safe disposal of electrical equipment. For Beckman Coulter products bearing this label please contact your dealer or local Beckman Coulter office for details on the take back program that will facilitate the proper collection, treatment, recovery, recycling and safe disposal of the device.



NONREFRIGERATED MODEL SPECIFICATIONS

Only values with tolerances or limits are guaranteed data. Values without tolerances are informative data, without guarantee.

Speed
Set speed 0 to 14 500 rpm (in 100-rpm increments)
or equivalent RCF
Time
Set time to 9 hr 59 min <i>or</i> continuous
Time display time remaining in run (timed run)
$or \infty$ and elapsed time (continuous run)
Acceleration
Deceleration
Ambient temperature range
Humidity restrictions
Dimensions
Width
Depth
Height, door closed
Height, door open
Weight
Clearances (sides and rear)
Electrical requirements 50 Hz, 230 VAC, 3 A; 60 Hz, 120 VAC, 5 A;
50/60 Hz, 100 VAC, 15 A
Motor
Electrical supply
Maximum heat dissipation into room
under steady-state conditions
Noise level 0.91 m (3 ft) in front of instrument ≤64 dBa
Installation (overvoltage) category
Pollution degree 2*

^{*}Normally only nonconductive pollution occurs, occasionally, however, a temporary conductivity caused by condensation must be expected.



REFRIGERATED MODEL SPECIFICATIONS

Only values with tolerances or limits are guaranteed data. Values without tolerances are informative data, without guarantee.

Speed
Set speed
Time
Set time to 9 hr 59 min <i>or</i> continuous
Time display
Temperature (continuous run)
Temperature setting
Operating range
Ambient temperature range
Humidity restrictions<95% (noncondensing)Acceleration10 acceleration profiles
<u>.</u>
Deceleration
Width
Depth
Height, door closed
Height, door open
Weight
Clearances (sides and rear)
Electrical requirements 50 Hz, 230 VAC, 5 A; 60 Hz, 120 VAC, 12 A;
50/60 Hz, 100 VAC, 15 A
Motor
Electrical supply
Maximum heat dissipation into room
under steady-state conditions
Noise level 0.91 m (3 ft) in front of instrument ≤64 dBa
Installation (overvoltage) category II
Pollution degree

 $^{^{\}ast}$ Temperature range depends on rotor in use and speed (see applicable rotor manual).

[†] Normally only nonconductive pollution occurs, occasionally, however, a temporary conductivity caused by condensation must be expected.

AVAILABLE ROTORS

		Refr	igerated	Nonre	frigerated		
Rotor Profile and Description		Max RPM	Max RCF* (× g)	Max RPM	Max RCF* (× g)	Max Capacity (mL)	Rotor Part Number/ Rotor Manual Number
	F2402H Fixed Angle 45° Angle	15 300	21 460	14 500	19 280	24 × 1.0/1.5	361171 GS-TB-021
	F3602 Fixed Angle 45° Angle	14 000	19 280	12 500	15 370	36 × 2.0/1.5	364600 GS-TB-006
	F0630 Fixed Angle 30° Angle	15 300	20 410	14 500	18 340	6 × 30	361231 GS-TB-014
	F0850 Fixed Angle 25° Angle	10 000	10 730	9 000	8 690	8 × 50	346640 GS-TB-003
	F0685 Fixed Angle 25° Angle	8 000	7 010	8 000	7 010	6 × 85	364650 GS-TB-008
	F1010 Fixed Angle 35° Angle	15 300	19 890	14 500	17 870	10 × 10	361221 GS-TB-007
	C0650 (Conical) Fixed Angle 25° Angle	9 500	9 380	9 000	8 420	6 × 50	364670 GS-TB-009
	C1015 (Conical) Fixed Angle 25° Angle	9 500	9 380	9 000	8 420	10 × 15	364680 GS-TB-011
	S4180 Swinging Bucket Four buckets	5 500	5 450	4 500	3 650	4 × 180	361109 GS-TB-004
	S2096 Microtiter	3 000	1 100	3 000	1 100	96 × 1.5/1.8	361111 GS-TB-005
	H6002 BioSafe Bowl Rotor	12 200	12 400	12 200	12 400	60 × 1.5/1.8 72 × 600 μL 84 × 250 μL	363000 GS30-TB-002

^{*} Values are rounded off.

Description

This section provides a brief physical and functional description of the Beckman Coulter Allegra 21 series, GS-15 series, and Spinchron 15 series centrifuges. The operating controls and indicators are also described; instructions for their use are in Section 3. Chemical compatibilities of materials listed in this manual can be found in Chemical Resistances (publication IN-175). Refer to the applicable rotor manuals for rotor descriptions.

INSTRUMENT FUNCTION AND SAFETY FEATURES

INSTRUMENT FUNCTION

The Beckman Coulter Allegra 21 series, GS-15 series, and Spinchron 15 series compact benchtop centrifuges generate centrifugal forces required for a wide variety of applications. Together with any of several Beckman Coulter rotors designed specifically for use in these centrifuges, the instrument applications include:

- Routine processing such as sample preparations, pelleting, extractions, purifications, concentrations, phase separations, receptor binding, and column centrifugations.
- Processing large numbers of small-volume samples in multiwell plates for concentrating tissue-culture cells, cloning and replicate studies, in-vitro cytoxicity studies, receptor binding, and genetic engineering experimentation.
- Rapid sedimentation of protein precipitates, large particles, and cell debris.
- Binding studies and separation of whole blood.
- · Cell isolation.

The centrifuges are microprocessor-controlled, providing interactive operation. The instrument design features a brushless three-phase drive system, automatic rotor overspeed identification system, program memory that can repeat the previously used run parameters for a given rotor, and a choice of acceleration/deceleration rates. The refrigerated models also have temperature control systems. User messages alert the operator to conditions that may need attention.

MODELS

The centrifuge is available in both nonrefrigerated and refrigerated models. See Figure 1-1. See the SPECIFICATIONS listed above for the operating differences between the refrigerated and nonrefrigerated models. Unless indicated otherwise, information in this manual is the same for both models.



Figure 1-1. The Allegra 21 and Allegra 21R Centrifuges. GS-15, GS-15R, Spinchron 15, and Spinchron 15R models are similar in appearance.

SAFETY FEATURES

The Allegra 21 series, GS-15 series, and Spinchron 15 series centrifuges have been designed and tested to operate safety indoors at altitudes up to 2000 m (6562 ft). Instrument safety features include the following:

- The door has dual electromechanical door-locking mechanisms to
 prevent operator contact with spinning rotors. When the door is
 closed it locks automatically. It can be unlocked only by pressing the
 [OPEN DOOR] key, and opened only when the power is on and the rotor
 is at rest. Two independent monitoring systems prevent the door from
 opening if the rotor is spinning.
- A steel barrier surrounds the rotor chamber to provide full operator protection.
- An overspeed system continuously monitors the rotor during centrifugation. The system includes a magnetic sensor on the drive motor and magnets imbedded in the rotors. Throughout the run, checks are made to ensure that the rotor does not exceed set speed.
- An imbalance detector monitors the rotor during the run, causing automatic shutdown if rotor loads are severely out of balance. At low speeds, an incorrectly loaded rotor can cause imbalance. Rotor instability can also occur if the centrifuge is moved while running, or if it is not resting on a level surface.
- Rubber pads on each of the centrifuge feet have been designed to minimize possible rotation in the event of a rotor mishap. For additional protection, an anchoring system is provided to secure the centrifuge in place. The anchoring system is designed to reduce the possibility of injury or damage which could result from instrument movement in the event of a major disruption.

NAME RATING PLATE

The name rating plate is affixed to the rear of the centrifuge. Check that the line voltage agrees with the voltage listed on this name rating plate before connecting the centrifuge. Always mention the serial number and the model number shown when corresponding with Beckman Coulter regarding your centrifuge.

CHASSIS

HOUSING

The centrifuge housing is made of sheet steel, finished with urethane paint. The control panel is covered by a protective overlay made of coated polycarbonate.

DOOR

The solid-sheet aluminum door is secured to the housing by solid shafts. A dual electromechanical door lock system prevents operator contact with spinning rotors and prevents run initiation unless the door is shut and latched. The door is locked when a run is in progress and can be opened only when the rotor is stopped. (A light-emitting diode [LED] on the [OPEN DOOR] key lights up when the door can be opened.) In the event of a power failure, the door lock can be manually tripped for sample recovery (see Section 4, TROUBLESHOOTING).

ROTOR CHAMBER

The rotor chamber is shown in Figure 1-2. The drive shaft, mounting plate, rubber boot surrounding the drive shaft, thermistor, and rotor detector are visible in the chamber bottom. A gasket system around the chamber opening assures sealing. (Instrument gaskets have not been designed as bioseals for aerosol containment.)

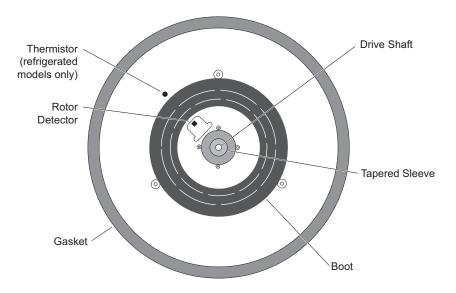


Figure 1-2. Interior View of the Rotor Chamber

DRIVE

The asynchronous three-phase direct-drive motor is brushless for clean, quiet operation. A tie-down screw is used to attach the rotor to the drive shaft. The resilient suspension ensures that loads will not be disturbed by vibration, and prevents damage to the drive shaft if an imbalance occurs during centrifugation. Maximum braking may be selected to reduce deceleration time, allowing fast processing of samples; alternately, delicate gradients may be preserved using slower deceleration.

TEMPERATURE SENSING AND CONTROL (refrigerated models only) With the power on, the temperature control system is activated when the door is closed. The run temperature can be set between -20 and $+40^{\circ}\text{C}$ in refrigerated models. If no set temperature is entered, the centrifuge automatically selects the last entered temperature. (For the first run of a new centrifuge, the instrument selects 20°C as its operating temperature.) A thermistor in the rotor chamber continuously monitors chamber temperature. The micro-processor calculates the required chamber temperature to maintain the selected rotor temperature.



In the unlikely event of a complete cooling system failure, the drive will switch off if the chamber temperature reaches 65°C. Restarting the centrifuge will not be possible until the chamber is cooled.

CONTROLS AND INDICATORS

POWER SWITCH

The power switch is located on the centrifuge back panel (see Figure 1-3). This two-position rocker switch (I, on; O, off) controls electrical power to the centrifuge.



The power must be turned on before the chamber door can be opened.


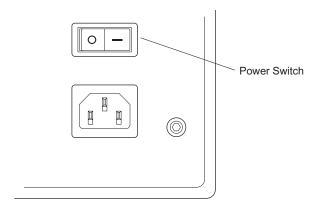



Figure 1-3. The Power Switch

CONTROL PANEL

The control panel (Figure 1-4), mounted at an angle on the centrifuge front for easy visibility and access, comprises touch keys—system keys and programming keys—and digital displays. The panel also contains an **IMBALANCE** light that flashes if rotor loads are severely out of balance.

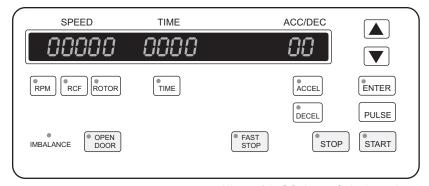

Allegra 21, GS-15, or Spinchron 15

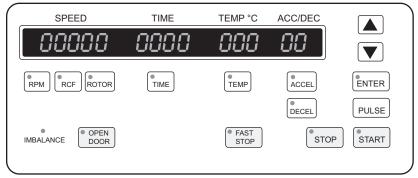


Allegra 21R, GS-15R, or Spinchron 15R

Figure 1-4. The Control Panels

System Keys

The centrifuge operation is controlled through the system keys. Each key (except the [PULSE] key) has an LED in the upper left corner that lights to indicate that the key can be activated.

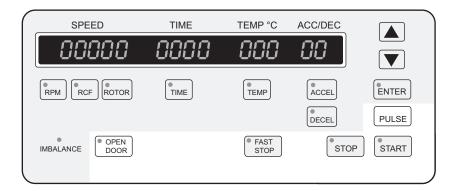

[START]

Pressing the [START] key causes the centrifuge run to begin. This key can also be used to abort a deceleration process and restart the centrifuge.

[STOP]

The [STOP] key can be pressed to end a run. The centrifuge decelerates to a complete stop according to the preselected deceleration curve. Deceleration can be terminated and the centrifuge restarted by pressing [START] again.

[FAST STOP]

Pressing the [FAST STOP] key causes the centrifuge to decelerate to a complete stop at the maximum rate. The deceleration cannot be interrupted; the centrifuge can only be restarted after the rotor stops and the door is opened and closed.

OPEN DOOR


Pressing the [OPEN DOOR] key unlatches the centrifuge door locks and allows the door to be opened. The centrifuge will accept this command *only when the rotor is completely stopped* and the [OPEN DOOR] key LED is lit.

[PULSE]

Pressing the [PULSE] key causes the installed rotor to accelerate up to the set speed for short-duration runs (as long as the key is pressed). Deceleration, at the maximum rate, begins when the key is released.

Program Keys

The program keys are used to set run parameters (a program consists of all of the parameters for a run). Except for the cursor and [ENTER] keys, program keys are located beneath the applicable digital displays, which show the parameters as they are input. Each key (except for the cursor keys) has an LED in the upper left corner that lights to indicate operational readiness. The LEDs also blink if an incorrect parameter is entered.

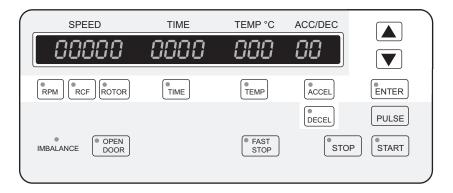

▲ (Cursor Keys)

The cursor keys are up and down arrow keys (\triangle and ∇), which can be pressed to increment values up or down when setting parameters.

[ENTER]

Parameter (speed, time, temperature, and acceleration or deceleration curve) changes made while a run is in progress must be verified by pressing the [ENTER] key.

[RPM]

When the [RPM] key is pressed the last digit in the SPEED display (0) flashes, indicating that the speed can be entered in increments of 100 revolutions per minute (rpm). After the run starts, the actual rpm of the rotor is displayed.

[RCF]

The [RCF] key can be used to select the speed setting by desired relative centrifugal field (RCF). The corresponding rpm is automatically calculated and displayed during the run. If the [RCF] key is pressed during the run, the RCF value is shown in the SPEED display.

[ROTOR]

The centrifuge memory contains a list of the rotors that can be used, together with default parameters for each rotor. When the [ROTOR] key is pressed the number of the rotor used in the previous run is shown on the **SPEED** display. The rotor list can be scrolled through, using the cursor keys, until the required rotor number appears.

[TIME]

The [TIME] key is used to select the run duration. When the [TIME] key is pressed, the last digit on the TIME display flashes, indicating that the time can be entered with the cursor keys.

- Timed run Run time up to 9 hours and 59 minutes can be set. If the minutes parameter exceeds 59, it is automatically converted into hours.
- Continuous run If a run time of less than 0 or more than 9 hours and 59 minutes is selected, continuous operation is activated. Time is not counted down, and the run will continue until the [STOP] or [FAST STOP] key is pressed.

[TEMP] (refrigerated models only)

The [TEMP] key is used to select run temperature on refrigerated model centrifuges. When the [TEMP] key is pressed, the TEMP $^{\circ}$ C display flashes, indicating that the temperature can be entered with the cursor keys. Temperature can be set between -20 and $+40^{\circ}$ C.


[ACCEL]

The [ACCEL] key is used to select acceleration rates that will protect delicate gradients. When the [ACCEL] key is pressed, the ACC/DEC display flashes, indicating that one of ten preset rates can be entered with the cursor keys. Acceleration rates are described in Table 3-1 (in Section 3).

[DECEL]

The [DECEL] key is used to select deceleration rates that will maintain optimum separation while protecting delicate gradients. When the [DECEL] key is pressed, the ACC/DEC display flashes, indicating that one of ten preset rates can be entered with the cursor keys. Deceleration rate selections are described in Table 3-1 (in Section 3).

Digital Displays

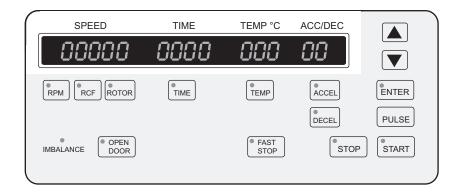

Digital displays indicate rotor speed, run time, rotor chamber temperature, and numbers that represent selected acceleration and deceleration profiles. When the power is turned on, they show the operating parameters of the most recent run performed before the power was turned off. The displays serve a dual purpose.

- When the run parameters are being set (the input mode), the displays show the set values (those selected by the operator). When a runparameter key (for example, [TIME] or [RPM]) is pressed, the appropriate display flashes to indicate that data can be entered.
- The *actual* (real-time) operating conditions of the centrifuge are displayed during the run, after [START] is pressed.



Error messages (see Section 4) also appear on the displays, when applicable.

SPEED

- *In input mode* the **SPEED** display shows the value of the parameter being set, depending on the programming key pressed ([RPM], [RCF], or [ROTOR]). For example, if the [ROTOR] programming key is pressed, a rotor number appears on the **SPEED** display.
- During centrifugation, the **SPEED** display shows the speed of the rotor in rpm. If the [RCF] key is pressed while the centrifuge is running, the RCF value is displayed.

TIME

- During a *timed run* (between 1 minute and 9 hours, 59 minutes), the **TIME** display begins counting down when the rotor starts to spin and continues the countdown until deceleration begins. The **TIME** display indicates the remaining run time in hours and minutes.
- During a *continuous run* (less than 0 or more than 9 hours, 59 minutes selected), countdown time is not displayed. Instead, the infinity (∞) symbol, indicating continuous operation, lights up and the **TIME** display shows time elapsed since the run start. After 9 hours and 59 minutes the timer will reset to 0 and continue counting elapsed time.

TEMP°C (refrigerated models only)

During standby (that is, the centrifuge is turned on but not spinning) and operation, the **TEMP°C** display shows the actual temperature inside the rotor chamber (± 2 °C at an ambient temperature of 20°C).

ACC/DEC

The ACC/DEC display shows the acceleration rate that was selected for the run. The deceleration curve number can be displayed by pressing the [DECEL] key.

Installation

This section contains instructions for installing and connecting the centrifuge. Check that required clearances and electrical power are available.



These centrifuges each weigh 50 kg/110.3 lb (nonrefrigerated model) or 70 kg/154.4 lb (refrigerated model.) DO NOT attempt to lift or move one of them without assistance from another person.

INSTALLING THE INSTRUMENT



Do not place the centrifuge near areas containing flammable reagents or combustible fluids. Vapors from these materials could enter the centrifuge air system and be ignited by the motor.

! WARNING				


Maintain a 7.6-cm (3-in.) clearance envelope around the centrifuge (secured with the anti-rotation kit) while it is running. No persons should be within this clearance boundary while the centrifuge is operating. Do not handle or store hazardous materials within the 30-cm (1-ft) area surrounding the centrifuge.

Position the centrifuge on a level surface, such as a sturdy table or laboratory bench that is able to support the weight of the centrifuge (refer to SPECIFICATIONS) and resist vibration.

- Locate the centrifuge in an area with sufficient ventilation to allow for heat dissipation.
- Check that there are 7.6-cm (3-in.) clearances at the sides and back of the centrifuge to ensure sufficient air circulation. Dimensions are shown in Figure 2-1. Additional clearance is required on the left side to allow access to the power switch. The centrifuge must have adequate air ventilation to ensure compliance to local requirements for vapors produced during operation.
- Ambient temperatures during operation should not be lower than 10°C (50°F) or higher than 35°C (95°F). Relative humidity should not exceed 95% (noncondensing).
- Use the anti-rotation kit to secure the centrifuge to the bench or table as described in publication GS-TB-016.



During transport between areas with varying temperatures, condensation may occur inside the centrifuge. Allow sufficient drying time before running the centrifuge.



The centrifuge is shipped with a cone-shaped plastic stabilizer installed in the rotor chamber to prevent damage to the drive motor and imbalance detector during transit. When installation of the centrifuge is complete, unscrew the tie-down bolt and remove the stabilizer. (Save the stabilizer to use during future relocation of the centrifuge.)

ELECTRICAL REQUIREMENTS

100-V instrument	90–100 VAC, 15 A, 50/60 Hz
120-V instrument (refrigerated)	108–132 VAC, 12 A, 60 Hz
120-V instrument (nonrefrigerated)	108–132 VAC, 5 A, 60 Hz
230-V instrument (refrigerated)	207–253 VAC, 5 A, 50 Hz
230-V instrument (nonrefrigerated)	207–253 VAC, 3 A, 50 Hz
Power cord	1.8-m (6-ft) power cord with grounded
	plug is supplied with the instrument

Make sure the voltage and frequency imprinted on the name rating plate affixed to the back of the centrifuge agree with the line voltage and frequency of the outlet used. (Refrigeration will not function properly if the frequency [Hz] does not match the name rating plate.) Plug in both ends of the centrifuge power cord. If there is any question about voltage, have a qualified service person measure it under load while the drive is operating.

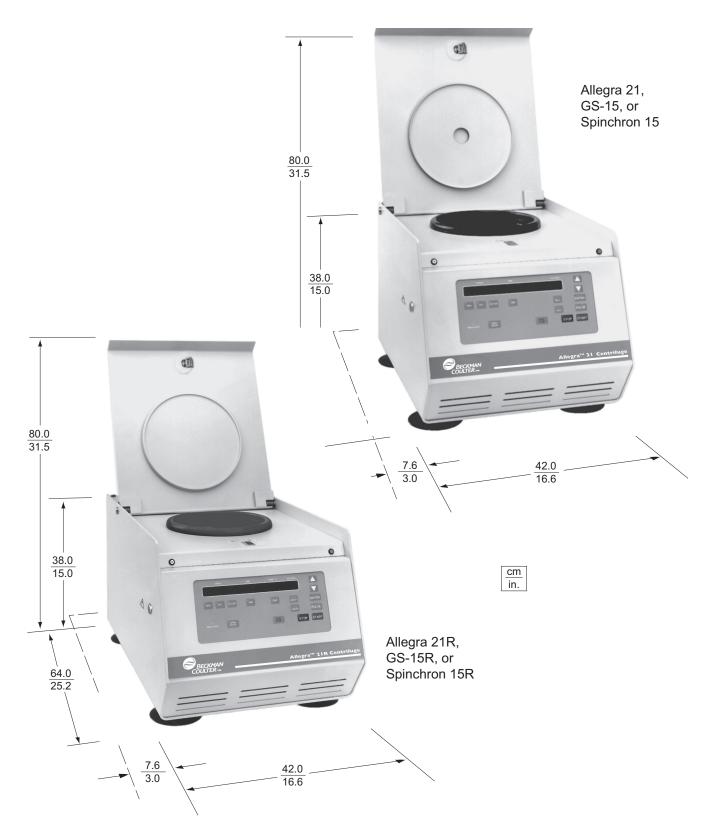


Figure 2-1. Dimensions of the Nonrefrigerated and Refrigerated Centrifuges

To ensure safety, the centrifuge should be wired to a remote emergency switch (preferably outside the room where the centrifuge is housed, or adjacent to the exit from that room), in order to disconnect the instrument from the main power source in case of a malfunction.



WARNING

To reduce the risk of electrical shock, this equipment uses a three-wire electrical cord and plug to connect the centrifuge to earth-ground. To preserve this safety feature:

- Make sure that the matching wall outlet receptacle is properly wired and earthgrounded. Check that the line voltage agrees with the voltage listed on the name rating plate affixed to the centrifuge.
- Never use a three-to-two wire plug adapter.
- Never use a two-wire extension cord or a two-wire non-grounding type of multipleoutlet receptacle strip.

TEST RUN



The centrifuge must be plugged in and the power switch turned to on position (I) before the door can be opened.

We recommend that you make a test run to ensure that the centrifuge is in proper operating condition following shipment. See Section 3 for instructions on operating the centrifuge.

After completing the test run, return the pre-addressed warranty card included with this literature. This will validate the centrifuge warranty and ensure your receipt of further information regarding new accessories and/or modifications as they become available.

Operation

This section contains operating procedures for the centrifuge, using any of the Beckman Coulter rotors designed for use in these centrifuges. Refer to the appropriate rotor manual for instructions on preparing the rotor for centrifugation. To prevent condensation, keep the centrifuge door closed and the power turned off (O) when the centrifuge is not in use.



WARNING

Normal operation may involve the use of solutions and test samples that are pathogenic, toxic, or radioactive. Operator error or tube failure may generate aerosols. Do not run potentially hazardous materials in this centrifuge unless all appropriate safety precautions are taken. Always use the appropriate rotors and adapters.

Handle all infectious samples according to good laboratory practices and methods to prevent the spread of disease. Ask your laboratory safety officer to advise you about the level of containment required for your application and about the proper decontamination or sterilization procedures to follow if fluids escape from containers. Biosafe containment should be used when Risk Group II materials (as identified in the World Health Organization Laboratory Biosafety Manual) are handled; materials of a higher group require more than one level of protection. Because spills may generate aerosols, observe proper safety precautions for aerosol containment.



The centrifuge must not be used in the vicinity of flammable liquids or vapors, and such materials should not be run in the centrifuge. During operation you should come within the 7.6 cm (3-in.) clearance envelope only to adjust instrument controls, if necessary. Never bring any flammable substances within the 30-cm (1-ft) area surrounding the centrifuge. Do not lean on the centrifuge or place items on the centrifuge while it is operating.

RUN PROCEDURE

The following detailed operating procedures are summarized at the end of this section. If you are an experienced user of this centrifuge, you can turn to the summary for a quick review of operating steps.

PREPARATION AND LOADING

For fast temperature equilibration, cool or warm the rotor to the required temperature before the run.



For high-speed runs at temperatures of 20°C or higher, prime the refrigeration system (refrigerated models) by running the instrument at 10°C for 5 to 10 minutes beforehand to prevent overheating.

- 1. Check the name rating plate for the correct voltage, then plug the power cord into the wall receptacle.
- 2. Press the power switch to on (I).
- 3. Press the [OPEN DOOR] key and lift the door up; it will remain in the open position.
- 4. Use the T-handle wrench to turn the rotor tie-down screw to the left (counterclockwise). Remove the tie-down screw.

5. Make sure that the tapered sleeve is in place at the base of the centrifuge drive shaft before installing the rotor (see Figure 3-1). The rotor rests on the sleeve while spinning, and will not operate properly if the sleeve is missing. Wipe the sleeve to be sure that it is clean and dry.




Figure 3-1. Tapered Sleeve Position



Do not drop the rotor onto the drive shaft. The shaft can be damaged if the rotor is forced sideways or dropped onto it. Install the rotor by centering it over the shaft and carefully lowering it straight down.

- 6. Install the rotor (see Figure 3-2) according to the instructions in the appropriate rotor manual. Always run the rotor with a balanced load. (If you are using a horizontal [swinging bucket] rotor, fill all four positions on the yoke of a swinging bucket rotor with buckets.)
- 7. Attach the tie-down screw to the drive shaft by turning it to the right (clockwise).
- 8. Use the T-handle wrench to tighten the tie-down screw on the shaft.



CAUTION

If the rotor is left in the centrifuge between runs, make sure the rotor is seated on the drive shaft and the tie-down screw is tight before each run. (Remove the rotor from the centrifuge if a long period between runs is anticipated.)

SWINGING BUCKET ROTOR FIXED ANGLE ROTOR Lower the yoke straight down onto the drive Lower the rotor straight down onto the drive shaft shaft Tighten the Tighten the tie-down screw tie-down screw clockwise onto clockwise onto the drive shaft the drive shaft Seat filled Attach the lid and buckets on tighten with the the yoke pins T-handle wrench

Figure 3-2. Installing a Rotor

9. If using a fixed-angle rotor with a lid, attach the lid. Tighten the lid with the T-handle wrench.

Fixed-angle rotors can be centrifuged without lids attached when longer tubes are used.

10. Close the centrifuge door and push firmly down on both sides of the door front until you hear a clicking (latching) sound.

ENTERING RUN PARAMETERS

When the power is applied for the initial use (no previous runs), default values will be displayed (see Figure 3-3). The centrifuge has an internal memory that stores previously used run parameters (or programs) for each rotor that has been centrifuged. After the initial use, the program (parameters) of the latest previous run will be displayed when power is applied

NOTE _____

A Program Library is provided at the back of this manual. You can use this chart to record the parameters of a run for later duplication of the run conditions.

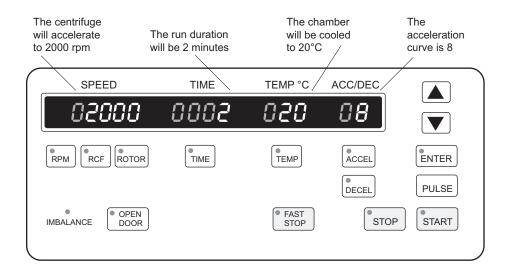


Figure 3-3. Default Parameters. The control panel shown is a refrigerated model; default values are the same for the nonrefrigerated model, except there is no temperature indication.

When run parameters for a rotor have been entered, as described below, they will be retained in the centrifuge memory and can be recalled by simply entering the rotor number. The recalled program can then be used for the current run or can be altered as required.

Selecting a Rotor Number

Each rotor that can be run in the centrifuge has a rotor number; the number is engraved on the rotor (and on the lid of fixed angle rotors). The centrifuge internal memory contains a list of all rotors that can be run in the centrifuge, together with acceptable run parameters for each rotor. If you enter an unauthorized rotor number then press the [START] key, an error message will be displayed and the run will be aborted shortly after the rotor starts spinning.

1. Press the [ROTOR] key.

A rotor number (the last rotor previously centrifuged) will appear on the **SPEED** display.

- 2. Press the ▲ or ▼ cursor key until the number of the rotor in use is displayed.
- 3. Press [ENTER].

Nominal parameter values (time, temperature, speed, acceleration and deceleration curves) for the selected rotor will be displayed. You can use these parameters or set new values for the run.

Setting Run Speed

Centrifuge speed can be set for up to the maximum rated speed of the selected rotor. Either revolutions per minute (rpm) or relative centrifugal field (RCF) can be used to select speed. During centrifugation, the **SPEED** display indicates the actual run speed of the rotor.

IIII NOTE

Use only the RPM mode to set run speeds for the H6002 bowl rotor. In the bowl rotor, RCF varies according to the tube in use, as indicated in the rotor manual (publication GS30-TB-002). If you use the RCF mode to set run speed, the centrifuge will select an RPM level based on the $r_{\rm max}$ of the largest tube, resulting in a speed too low to achieve the required RCF in the shorter tubes. Also note that the control panel will display the RCF calculated for the $r_{\rm max}$ of the 1.8-or 1.5-mL tube, which will not accurately represent the RCF for shorter tubes. Refer to the rotor manual for the RCF values of shorter tubes.

Setting RPM

1. Press the [RPM] key.

The last digit on the **SPEED** display (0) will flash, indicating that the rpm can be entered (in 100-rpm increments) with the cursor keys.

2. Press the \triangle or ∇ cursor key until the required rpm is displayed.

The corresponding RCF will be automatically calculated by the centrifuge, but the rpm value will be displayed during the run. (You can check the RCF during the run by pressing the [RCF] key while the centrifuge is running.)

Setting RCF

1. Press the [RCF] key.

The last digit on the **SPEED** display (0) will flash, indicating that the RCF can be entered.

2. Press the \triangle or ∇ cursor key until the required RCF is displayed.

The corresponding rpm will be automatically calculated and the centrifuge will run at the calculated speed. The rpm value will be displayed during the run. (You can check the RCF during the run by pressing the [RCF] key while the centrifuge is running.)

Setting Run Time

Run time can be set for either a timed run or continuous operation.

- Timed run Time can be set for up to 9 hours and 59 minutes (if the minutes parameter entered exceeds 59, it is automatically converted into hours). During centrifugation, the TIME display begins counting down when the rotor starts to spin and continues the count-down until deceleration begins. The TIME display shows the time remaining in the run, in hours and minutes. When the time display reaches zero, the run ends.
- Continuous run If a run time of less than 0 or more than 9 hours and 59 minutes is selected, continuous operation is activated. Time is not counted down during continuous operation; instead, the infinity (∞) symbol, indicating continuous operation, lights up and time elapsed since the run start is displayed. The run will continue until the [STOP] or [FAST STOP] key is pressed.
- 1. Press the [TIME] key.

The last digit on the **TIME** display will flash, indicating that the time can be entered with the cursor keys.

2. Press the \triangle or ∇ cursor key until desired run duration is displayed.

Setting Run Temperature (refrigerated models only)

Run temperature can be set between -20 and +40°C.



Temperatures may vary slightly between instruments. If sample temperature is crucial, test temperature settings on your instrument using water samples.

1. Press the [TEMP] key.

The **TEMP°C** display will flash, indicating that the temperature can be entered with the cursor keys.

2. Press the ▲ or ▼ cursor key until the desired run temperature is displayed.



For runs at other than room temperature, refrigerate or warm the rotor beforehand for fast equilibration. For low-temperature runs, precool the centrifuge by running a 30-minute cycle at the desired temperature (with a precooled rotor installed) with the speed set at about 2000 rpm.

Setting Acceleration Rate

The [ACCEL] key is used to select acceleration rates that will protect delicate gradients. When the [ACCEL] key is pressed, the ACC/DEC display flashes, indicating that one of the 10 preset acceleration rates can be entered with the cursor keys. The selected rate will depend on the type of run you are performing. For pelleting runs, where sample mixing is not a concern, maximum acceleration can be used. However, if delicate gradients are being run, a lower setting may be needed. Acceleration rates are listed in Table 3-1.

Table 3-1. Acceleration/Deceleration Times (in minutes:seconds). Times are approximate; actual times will vary depending on rotor load.

		Refrigerat	ed Models		Nonrefrigerated Models			
	Horizontal Rotors (5 500 rpm)*		Fixed Angle Rotors (15 300 rpm)		Rot	contal tors rpm)*	Ro	Angle tors 0 rpm)
Curve	Accel	Decel	Accel	Decel	Accel	Decel	Accel	Decel
9	0:54	0:40	0:47	1:04	0:25	0:23	0:44	0:47
8	0:54	0:29	1:20	1:17	0:27	0:24	1:06	1:09
7	0:56	1:03	2:29	2:28	0:29	0:26	2:03	2:12
6	1:40	1:39	4:55	4:52	0:30	0:30	4:11	4:12
5	2:30	2:26	7:39	7:17	1:04	1:07	6:13	6:14
4	3:18	3:11	10:02	9:42	1:08	1:11	8:07	8:05
3	4:54	4:48	15:16	14:33	2:13	2:18	11:12	11:26
2	9:41	9:35	29:07	30:56	4:31	4:34	23:17	23:20
1	14:40	14:11	45:56	46:16	12:03	12:17	40:00	40:16
0	14:40	14:11	61:01	46:16	12:03	12:17	40:00	40:16

^{*}Maximum speed for the S2096 microtiter rotor is 3000 rpm; acceleration and deceleration times will decrease accordingly.

1. Press the [ACCEL] key.

The ACC/DEC display will flash, indicating that the selected rate number can be entered with the cursor keys.

2. Press the \triangle or ∇ cursor key until the required number is displayed.

Setting Deceleration Rate

The [DECEL] key is used to select deceleration rates that will maintain optimum separation. When the [DECEL] key is pressed, the ACC/DEC display flashes, indicating that one of the ten preset deceleration rates can be entered with the cursor keys. The selected rate will depend on the type of run you are performing. For pelleting runs, where sample mixing is not a concern, maximum brake can be used. However, if delicate gradients are being run, a lower brake setting may be needed. Deceleration rates are listed in Table 3-1.

1. Press the [DECEL] key.

The ACC/DEC display will flash, indicating that the selected number can be entered with the cursor keys.

2. Press the ▲ or ▼ cursor key until the required number is displayed.

STARTING A RUN


The run can be started using the parameters in memory from a previous run, or using new or changed parameters that you enter using the procedure described above.

- 1. Check that all parameters are correct and the door is shut and latched.
- 2. Press the [ENTER] key, then the [START] key.


As the run begins, the instrument rotor identification system compares the rotor in the chamber to the entered rotor number and the speed entered. An incorrect rotor identification, or set speed greater than the *rotor's maximum permitted speed*, will result in an error code and the centrifuge will shut down. (See Section 4, TROUBLESHOOTING, for information on error codes.) The error must be cleared and an appropriate speed entered before the centrifuge can be started. Throughout the run, checks are made to ensure that the rotor does not exceed set speed.

• The **SPEED** display indicates the rotor speed in rpm. (The RCF can be checked by pressing the [RCF] key.)

• A blinking LED at the bottom of the **TIME** display indicates that the run is in progress. This display also shows the time remaining in the run (or ∞ and elapsed time for continuous operation).

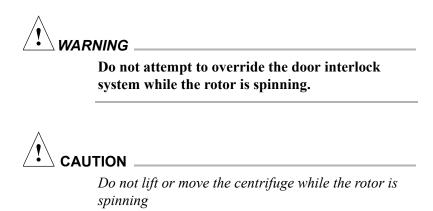

CHANGING PARAMETERS DURING A RUN While a run is in progress, run parameters (speed, time, temperature, and acceleration or deceleration rate) can be altered without stopping the run. Run duration can also be changed from continuous to a specified time period, or from a specified time period to continuous.



Use the program keys as described under ENTERING RUN PARAMETERS, above, to change parameters. Parameter changes made during a run must be verified by pressing the [ENTER] key. For example, to change run speed during centrifugation:

1. Press the [RPM] key.

The last digit on the **SPEED** display will flash, indicating that the rpm can be raised or lowered with the cursor keys.

- 2. Press the \triangle or ∇ cursor key until the required rpm is displayed.
- 3. Press the [ENTER] key.

The current rpm value will be displayed, changing to the new value as the rotor accelerates or decelerates to the new speed selected. The corresponding RCF will be automatically calculated by the centrifuge.

STOPPING A RUN

A timed run will end automatically when the **TIME** display counts down to zero. To end a run in progress for any reason:

1. Press the [STOP] key for normal deceleration as selected by the deceleration curve.

(or)

Press the [FAST STOP] key for deceleration at the maximum rate (see Table 3-1).

IIII NOTE

If you press [FAST STOP] the deceleration process cannot be interrupted; the centrifuge can be restarted only after the rotor comes to a complete stop and the door is opened and closed.

2. *After the rotor stops spinning* and the [OPEN DOOR] light comes on, press the [OPEN DOOR] key to release the door latches, then open the door.

IIII NOTE

To prevent chamber icing, use a sponge to wipe condensation out of the chamber bowl between runs.

UNLOADING



When you remove the rotor, make sure that the tapered sleeve from the centrifuge drive shaft does not come out with the rotor. If the tapered sleeve is inside the rotor drive hole, remove it and put it back on the drive shaft (see Figure 3-1).

After completing a run, unload the rotor following the instructions in the applicable rotor manual.




If disassembly reveals evidence of leakage, you should assume that some fluid escaped the rotor. Appropriate decontamination procedures should be applied to the centrifuge and accessories.


SUMMARY OF RUN PROCEDURES

For runs at other than room temperature, refrigerate or warm the rotor beforehand for fast equilibration. For low-temperature runs, precool the centrifuge by running a 30-minute cycle (with a precooled rotor installed) at the desired temperature with the speed set at 2000 rpm.

- 1. Press the POWER switch to on (I). Open the centrifuge door (press the [OPEN DOOR] key and lift the door up).
- 2. Make sure that the tapered sleeve is in place at the base of the centrifuge drive shaft before installing the rotor. The rotor will not operate properly if the sleeve is missing.
- 3. Install the rotor according to the instructions in the applicable rotor manual. *Always run the rotor with a balanced load*.
- 4. Close the centrifuge door and push firmly down on it until you hear the latch engage.
- 5. Enter run parameters:
 - Select a rotor number [ROTOR], ▲ or ▼, [ENTER]
 - Set run speed [RPM], \triangle or ∇ ; or [RCF], \triangle or ∇
 - Set run duration [TIME], ▲ or ▼
 - Set run temperature [TEMP], ▲ or ▼
 - Select acceleration rate (0 through 9)— [ACCEL], ▲ or ▼
 - Select deceleration rate (0 through 9)—[DECEL], ▲ or ▼

6. Check that all parameters are correct and the door is shut and latched, then press [ENTER], then [START].





- 7. Wait for the set time to count down to zero, or end the run by pressing either the [STOP] key or the [FAST STOP] key.
- 8. *After the rotor stops spinning* and the [OPEN DOOR] light comes on, press the [OPEN DOOR] key to release the door latch; open the door.
- 9. Unload the rotor according to instructions in the applicable rotor manual.



If disassembly reveals evidence of leakage, you should assume that some fluid escaped the rotor. Appropriate decontamination procedures should be applied to the centrifuge and accessories.

Troubleshooting

This section lists possible malfunctions, together with probable causes and corrective actions required. Maintenance procedures are contained in Section 5. For any problems not covered here contact your Beckman Coulter Field Service representative.



It is your responsibility to decontaminate the centrifuge, as well as any rotors and accessories, before requesting service by Beckman Coulter Field Service representatives.

USER MESSAGES



CAUTION

If the message SEr appears on the display, do not press any keys while the message is displayed. Turn the centrifuge power off (O) and back on (1) to clear the message. This message indicates that you have inadvertently accessed the service mode. Pressing any keys while in this mode could erase the centrifuge memory and critically interfere with future operation.

If a problem occurs during operation, the rotor will decelerate to a stop and an error code will appear on the **SPEED** display. Messages may result from incorrect input or from an equipment malfunction. Refer to Table 4-1

Table 4-1. Error Message Chart.

If the recommended action does not correct the problem, call Beckman Coulter Field Service.

Error Number	Problem	Result	Recommended Action
1 through 23, 25 and 26, 28 through 30 32, 36, 39 and 40, 44 through 60, 63 through 68	Microprocessor or mechanical malfunction	Deceleration to full stop; run cannot be restarted	After rotor comes to a complete stop, turn the power off (O), then back on (I) to reset.
23 and 24, 27, 31, 33 through 35, 37 and 38, 41 through 43, 62	Microprocessor or mechanical malfunction	Deceleration to full stop; run cannot be restarted	After rotor comes to a complete stop, open and close the centrifuge door, then restart.
69 through 77	Microprocessor malfunction	Run cannot start until error is cleared	Turn the power off (O), then back on (I) to reset.
78 through 80	Error during closing of door	Run cannot start	 Remove debris in latch Close lid quickly. Turn the power off (O), then back on (I) to reset.
81	"Door open" detected during run	Maximum deceleration to full stop	After rotor comes to a complete stop, shut the centrifuge door, turn the power off (O), then back on (I) to reset.
82, 83	Door does not open	_	See EMERGENCY ACCESS, below
84	Heat sink overtemperature	Deceleration to full stop	Check that ambient temperature is within a the limits shown in SPECIFICATIONS.
85 through 87	Rotor chamber overtemperature (refrigerated models)	Deceleration to full stop	Check air inlets and exhausts for obstructions. After the motor has cooled, restart. If the problem persists, call Beckman Coulter Field Service.
90 through 96	Temperature sensor malfunction (refrigerated models)	Maximum deceleration to full stop	Turn the power off (O), then back on (I) to reset.
98	Rotor not recognized	Maximum deceleration to full stop	Check that the installed rotor is usable in the centrifuge. If incorrect, install an authorized rotor; if rotor is authorized and problem persists, call Beckman Coulter Field Service.
99	Rotor recognized but incorrect	Maximum deceleration to full stop	Input correct parameters for the rotor in use, then restart.

to determine the nature of the problem and recommended actions. If you are unable to correct the problem, call your Beckman Coulter Field Service representative. To help diagnose and correct the problem, try to gather as much information about the situation as you can:

- Write down the error number that appears on the display.
- Note the operating situation when the error occurred (rotor in use, speed, load type, etc.).
- Note any unusual environmental and/or operating conditions (ambient temperature, voltage fluctuations, etc.).
- Add any other information you think may be helpful.

OTHER POSSIBLE PROBLEMS

Possible malfunctions that may not be indicated by diagnostic messages are described in Table 4-2, along with probable causes and corrective actions required. Possible causes for each problem are listed in the probable order of occurrence. Perform the recommended corrective action in sequence, as listed. If you are unable to correct the problem, call your Beckman Coulter Field Service representative.

EMERGENCY ACCESS

If the facility power fails only momentarily, the centrifuge will resume operation when power is restored and the rotor will return to set speed. However, if the rotor comes to a complete stop you will have to restart the run when the power is restored. In the event of an extended power failure, it may be necessary to trip the door-locking mechanism manually to remove the rotor and retrieve your sample (see Figure 4-1).

1. Turn the power switch to off (O) and disconnect the power cord from the main power source.

NAF	RNING
	Never attempt to override the door interlock system while the rotor is spinning.

Table 4-2. Troubleshooting Chart

Problem	Problem/Result	Recommended Action
Imbalance LED lights and rotor decelerates to stop	Rotor is out of balance	Check to be sure the rotor is in good condition and is loaded symmetrically around the center of rotation, with containers of equal weight and density (within 6 grams) opposite each other.
	Centrifuge is misaligned (tilted)	2. Align the centrifuge on the bench or table.
	Centrifuge was moved during operation	After the rotor comes to a complete stop, open and close the centrifuge door, then restart.
	Drive error (mechanical damage)	Call Beckman Coulter Field Service.
Rotor cannot achieve set speed	Line voltage below rating	Have a qualified service person measure line voltage while the instrument is operating.
	2. Electrical failure	Make sure both ends of the power cord are securely connected; call Beckman Coulter Field Service.
	3. Motor failure	3. Call Beckman Coulter Field Service.
Door will not open	 Rotor spinning Power not on Source power failure Latch stuck 	 Wait until the rotor stops. Plug in the power cord; turn power on (I). See EMERGENCY ACCESS, below. See EMERGENCY ACCESS, below.
Displays are blank	Power not on Electrical failure Fuse blown	Plug in the power cord; turn power on (I). Make sure both ends of the power cord are securely connected; call Beckman Coulter Field Service. Call Beckman Coulter Field Service.
TEMP °C display flashes (refrigerated models)	Chamber temperature is >25°C higher than selected temperature	Precool rotors before running at low temperatures. Precool rotor chamber by running a 30-minute cycle at the desired temperature with the speed set at about 2000 rpm. If a lower temperature deviation alert is required, contact Beckman Coulter Field Service.
Chamber does not reach selected temperature (refrigerated models)	Centrifuge cannot maintain selected temperature for rotor in use at speed selected	Refer to appropriate rotor manual for temperature and speed requirements. Also, precool rotors before running at low temperatures. Precool rotor chamber by running a 30-minute cycle at the desired temperature with the speed set at 2000 rpm.

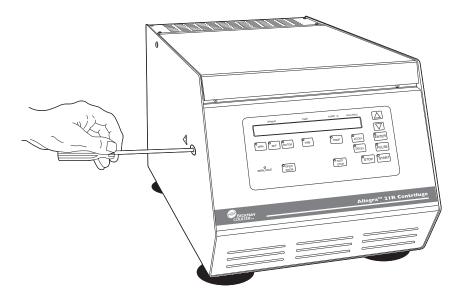


Figure 4-1. Emergency Door Release

- 2. Make sure that the rotor is not spinning.
- 3. Insert a socket-head wrench in the emergency door release screw on the centrifuge side panel (see Figure 4-1).
- 4. Rotate the screw clockwise until you hear a "click" or the door pops open.
- 5. Remove the wrench.

If the rotor is still spinning, close the door and wait until it stops before attempting to remove it.



Care and Maintenance

For maintenance not covered in this manual, contact your local Beckman Coulter Field Service representative. User messages are discussed in Section 4, TROUBLESHOOTING. Refer to the applicable rotor manual and to Chemical Resistances (publication IN-175) for instructions on the care of rotors and their accessories.



It is your responsibility to decontaminate the centrifuge, as well as any rotors and accessories, before requesting service by Beckman Coulter Field Service representatives.



Any maintenance procedure or servicing of this equipment that requires removal of any covers can expose parts which involve the risk of electric shock or personal injury. Make sure that the power switch is off (O) and the centrifuge is disconnected from the main power source, and refer such servicing to qualified service personnel.

Do not use alcohol or other flammable substances in or near operating centrifuges.

MAINTENANCE

PREVENTIVE MAINTENANCE

The following procedures should be performed regularly to ensure continued performance and long service life of the centrifuge.

- Regularly inspect the interior of the rotor chamber for accumulations
 of sample, dust, or glass particles from broken sample tubes. Clean as
 required (see CLEANING, below), as these accumulations can result in
 rotor vibrations.
- Regularly check the air intake and exhaust vents for obstructions. Keep vents clear and clean.
- Use a sponge to wipe condensation out of the chamber bowl between runs to prevent chamber icing (refrigerated models). If chamber icing occurs, defrost before use.
- To prevent the rotor from sticking, lubricate the drive shaft with Spinkote at least once a month, and after each cleaning.

REPLACING THE ROTOR CHAMBER GASKET

If the gasket (961806) around the rotor chamber opening becomes damaged or worn, replace it as follows. (See Figure 5-1.)

- 1. Remove the gasket by pulling it up and away from the opening.
- 2. Install the new gasket by positioning the groove in the gasket over the rim of the opening.
- 3. Press the gasket around the opening so that the rim is seated in the gasket groove.

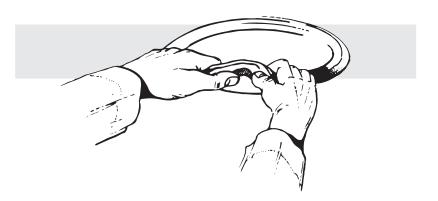


Figure 5-1. Replacing the Rotor Chamber Gasket

CLEANING

Frequent cleaning is recommended to prolong the life of the centrifuge. Always clean up spills when they occur to prevent corrosives or contaminants from drying on component surfaces.

- To prevent accumulations of sample, dust, and/or glass particles from broken sample tubes, keep the interior of the rotor chamber clean and dry by frequent wiping with a cloth or paper towel.
- Clean the drive shaft, shaft cavity, threads, and the tie-down screw at least once a week using a mild detergent such as Beckman Solution 555TM and a soft brush. Dilute the detergent 10 to 1 with water. Rinse thoroughly and dry completely. Lubricate the drive shaft with Spinkote after cleaning.
- Wash the bowl using a mild detergent such as Solution 555. Rinse thoroughly and dry completely.
- Clean the centrifuge case and door by wiping with a cloth dampened with Solution 555. Do not use acetone or other solvents.



Before using any cleaning or decontamination methods except those recommended by the manufacturer, users should check with the manufacturer that the proposed method will not damage the equipment.

TUBE BREAKAGE

If a glass tube breaks, and all the glass is not contained in the bucket or rotor, it will be necessary to thoroughly clean the interior of the chamber bowl.



Be careful when examining or cleaning the sealing gasket or chamber, as sharp glass fragments may be embedded in their surfaces.

- Examine the gasket to make sure that no glass particles are retained in it. Carefully remove any glass particles that may remain.
- Carefully wipe away any glass particles that remain in the bowl.

DECONTAMINATION

If the instrument and/or accessories are contaminated with radioactive or pathogenic solutions, perform appropriate decontamination procedures. Refer to *Chemical Resistances* (IN-175) to be sure the decontamination method will not damage any part of the instrument.


STERILIZATION AND DISINFECTION

The centrifuge is finished with urethane paint. Ethanol (70%)* may be used on this surface. See *Chemical Resistances* for more information regarding chemical resistance of centrifuge and accessory materials.

While Beckman Coulter has tested these methods and found that they do not damage the centrifuge, no guarantee of sterility or disinfection is expressed or implied. When sterilization or disinfection is a concern, consult your laboratory safety officer regarding proper methods to use.

STORAGE AND TRANSPORT

STORAGE



Before storing a centrifuge for an extended period, return it to its original shipping container to protect it from dust and dirt. Reinstall the plastic stabilizer (removed at time of centrifuge installation) to prevent damage to the drive rotor and imbalance detector. Temperature and humidity conditions for storage should meet the environmental requirements described under SPECIFICATIONS.

RETURNING A CENTRIFUGE

Before returning a centrifuge or accessory for any reason, prior permission (a Returned Goods Authorization form) must be obtained from Beckman Coulter, Inc. Contact your local Beckman Coulter office to obtain the RGA form and for packaging and shipping instructions.

^{*} Flammability hazard. Do not use in or near operating centrifuges.

To protect our personnel, it is the customer's responsibility to ensure that all parts are free from pathogens and/or radioactivity. Sterilization and decontamination must be done before returning the parts.

All parts must be accompanied by a signed note, plainly visible on the outside of the box, stating that they are safe to handle and that they are not contaminated with pathogens or radioactivity. Failure to attach this notification will result in return or disposal of the items without review of the reported problem.

SUPPLY LIST

Refer to the applicable rotor manual for materials and supplies needed for rotors.



Publications referenced in this manual can be obtained by calling Beckman Coulter at 1-800-742-2345 in the United States, or by contacting your local Beckman Coulter office.

Contact Beckman Coulter Sales (1-800-742-2345 in the United States; worldwide offices are listed at the back of this manual) for information about ordering parts and supplies. For your convenience, a partial list is given below.

REPLACEMENT PARTS

Power cord (60-Hz)	39097
Power cord (50-Hz)	51130
Rotor chamber gasket96	51806
Rotor tie-down screw	51367
T-handle wrench	51371

SUPPLIES

Spinkote lubricant (2 oz)	306812
Silicone vacuum grease (1 oz)	335148
Beckman Solution 555 (1 qt)	39555

Program Library

Record the program parameters on the chart below as a quick reference when duplicating run conditions. Refer to Section 3 of this manual for the numbers representing acceleration and deceleration (ACCEL/DECEL) rates.

December				Spe	eed	Time	Taman	ACCEL	DECEL
Program Number	User	Date	Purpose	RPM	RCF	Time (hrs/min)	Temp (°C)	Rate	Rate

Drogram				Speed		Time	Tomp	ACCEL	DECEL
Program Number	User	Date	Purpose	RPM	RCF	(hrs/min)	Temp (°C)	Rate	Rate

ALLEGRA 64R, AVANTI 30, GS-15 SERIES, ALLEGRA 21 SERIES AND SPINCHRON 15 SERIES CENTRIFUGE WARRANTY

Subject to the exceptions and upon the conditions specified below, Beckman Coulter agrees to correct, either by repair, or, at its election, by replacement, any defects of material or workmanship which develop within one (1) year after delivery of the Avanti 64R, Avanti 30, Allegra 21, GS-15, or Spinchron 15 series centrifuge (the product), to the original Buyer by Beckman Coulter or by an authorized representative provided that investigation and factory inspection by Beckman Coulter discloses that such defect developed under normal and proper use.

Some components and accessories by their nature are not intended to and will not function for as long as one (1) year. A complete list of such components or accessories is maintained at the factory and at each Beckman Coulter District Sales Office. The lists applicable to the products sold hereunder shall be deemed to be part of this warranty. If any such component or accessory fails to give reasonable service for a reasonable period of time, Beckman Coulter will repair or, at its election, replace such component or accessory. What constitutes either reasonable service and a reasonable period of time shall be determined solely by Beckman Coulter.

REPLACEMENT

Any product claimed to be defective must, if requested by Beckman Coulter, be returned to the factory, transportation charges prepaid, and will be returned to Buyer with the transportation charges collect unless the product is found to be defective, in which case Beckman Coulter will pay all transportation charges.

Beckman Coulter makes no warranty concerning products or accessories not manufactured by it. In the event of failure of any such product or accessory, Beckman Coulter will give reasonable assistance to the Buyer in obtaining from the respective manufacturer whatever adjustment is reasonable in light of the manufacturer's own warranty.

CONDITIONS

Beckman Coulter shall be released from all obligations under all warranties either expressed or implied, if the product(s) covered hereby are repaired or modified by persons other than its own authorized service personnel, unless such repair in the sole opinion of Beckman Coulter is minor, or unless such modification is merely the installation of a new Beckman Coulter plug-in component for such product(s).

DISCLAIMER

IT IS EXPRESSLY AGREED THAT THE ABOVE WARRANTY SHALL BE IN LIEU OF ALL WARRANTIES OF FITNESS AND OF THE WARRANTY OF MERCHANT-ABILITY AND THAT BECKMAN COULTER, INC. SHALL HAVE NO LIABILITY FOR SPECIAL OR CONSEQUENTIAL DAMAGES OF ANY KIND WHATSOEVER ARISING OUT OF THE MANUFACTURE, USE, SALE, HANDLING, REPAIR, MAINTENANCE, OR REPLACEMENT OF THE PRODUCT.



Beckman Coulter, Inc. • 250 S. Kraemer Blvd. • Brea, California 92821 Sales and Service: 1-800-742-2345 • Internet: www.beckmancoulter.com

