

20000006451

MIDI\_MAXI\_032016

# IKA®

## IKA® MIDI MR 1 digital IKA® MAXI MR 1 digital



[www.imlab.eu](http://www.imlab.eu)

info@imlab.be - Tél. : +32 (0)16 73 55 72

**imLab**

[www.imlab.eu](http://www.imlab.eu)

info@imlab.fr - Tél. : +33 (0)3 20 55 19 11

Imlab sprl - Oude Vijvers, 1  
3370 Boutersem - Belgique

Imlab sarl - Centre d'Affaires de l'Horlogerie  
48 rue des Canoniers - 59000 Lille - France






## Contents

	Page
Declaration of conformity	11
Explication of warning symbols	11
Safety instructions	11
Correct use	13
Unpacking	13
Commissioning	13
Interface and output	14
Maintenance and cleaning	16
Error codes	16
Accessories	16
Technical data	17
Warranty	17

## Declaration of conformity

We declare under our sole responsibility that this product is in compliance with the regulations 2014/35/EU, 2014/30/EU and 2011/65/EU and conforms to the standards or normative documents: EN 61010-1, EN 61010-2-051, EN 61326-1, EN 60529 and EN ISO 12100.

## Explication of warning symbols

 <b>DANGER</b>	Indicates an (extreme) hazardous situation, which, if not avoided, will result in death, serious injury.
 <b>WARNING</b>	Indicates a hazardous situation, which, if not avoided, can result in death, serious injury.
 <b>CAUTION</b>	Indicates a potentially hazardous situation, which, if not avoided, can result in injury.
 <b>NOTICE</b>	Indicates practices which, if not avoided, can result in equipment damage.
 <b>NOTICE</b>	Note the hazards of magnetism!

## Safety instructions

### **General information:**

- **Read the operating instructions completely before starting up and follow the safety instructions.**
- Keep the operating instructions in a place where they can be accessed by everyone.
- Ensure that only trained staff work with the device.
- Follow the safety instructions, guidelines, occupational health and safety and accident prevention regulations.
- Socket must be earthed (protective ground contact).
- The socket for the mains cord must be easily accessible.
- The feet of the device must be clean and undamaged.
- Check the device and accessories for damage before each use them. Do not use damaged components.
- Do not operate the device in explosive atmospheres, with hazardous substances or under water.
- The device may heat up when in use.

- Do not move or transport the device when it is operating or connected to the power supply.
- Safe operation is only guaranteed with the accessories described in the "**Accessories**" chapter.
- Always disconnect the plug before attaching accessories.
- The device can only be disconnected from the mains supply by pulling out the mains plug or the connector plug.
- The device can only be opened by technical experts, even during repair. The device must be unplugged from the power supply before opening. Live parts inside the device may still be live for some time after unplugging from the power supply.



#### NOTICE

Effects of the magnetic field have to be taken into account (e.g. data storage media, cardiac pacemakers ...).

- The working plate can heat up due to the action of the drive magnets at high motor speeds.
- The centre of gravity of the assembly must lie within the surface on which it is set up.
- It may be possible for wear debris from rotating accessory parts to reach the material being processed.
- When using PTFE-coated magnetic bars, the following has to be noted: Chemical reactions of PTFE occur in contact with molten or solute alkali metals and alkaline earth metals, as well as with fine powders of metals in groups 2 and 3 of the periodic system at temperatures above 300 °C - 400 °C. Only elementary fluorine, chlorotrifluoride and alkali metals attack it; halogenated hydrocarbons have a reversible swelling effect.

(Source: *Römpps Chemie-Lexikon* and "*Ulmann*", Volume 19)

#### **For protection of the user:**



#### WARNING

Wear your personal protective equipment in accordance with the hazard category of the media

to be processed. There may be a risk from:

- splashing and evaporation of liquids
- ejection of parts
- release of toxic or combustible gases.



#### DANGER

Only process media that will not react dangerously to the extra energy produced through processing. This also applies to any extra energy produced in other ways, e.g. through light irradiation.



#### DANGER

Process pathogenic materials only in closed vessels under a suitable fume hood. Please contact **IKA®**

if you have any questions.



#### WARNING

Beware of hazards due to:

- flammable materials
- incorrect container size
- overfilling of media
- unsafe condition of container.

#### **For protection of the device and accessories:**

- Set up the device in a spacious area on an even, stable, clean, non-slip, dry and fireproof surface.
- The voltage stated on the type plate must correspond to the mains voltage.
- Removable parts must be refitted to the device to prevent the infiltration of foreign objects, liquids etc..
- Protect the device and accessories from bump and impact.
- Do not cover the device, even partially e.g. with metallic plates or film. This may result in overheating.

#### **Performing trials:**



#### NOTICE

Reduce the speed if:

- the medium splashes out of the vessel
- the device is not running smoothly
- dynamic forces start to cause the device and/or the vessels placed on it to move around.
- Make certain that the device is set at the lowest speed (left hand position) before commissioning; otherwise, the device will start to run at the speed set in last operation. Gradually increase the speed.
- After an interruption in the power supply or a mechanical interruption during working process, the device will restart automatically.

## Correct use

The **IKA® MIDI MR 1 digital** and **MAXI MR 1 digital** is a magnetic stirrer without heating function. The devices are suitable for stirring and mixing liquid substances up to 50 liter (**MIDI MR1 digital**) and 150 liters (**MAXI MR1 digital**). The built-in stirring drive permits the stirring of substances with the aid of a magnetic stirring bar in the vessel. The mixing intensity is dependent on the motor speed and the size of the magnetic bar.

- **Use:**

- for stirring and mixing liquids.

Intend use: Tabletop device

- **Range of use (indoor use only):**

- Laboratories
- Pharmacies
- Schools
- Universities

This device is suitable for use in all areas except:

- Residential areas.
- Areas that are connected directly to a low-voltage supply network that also supplies residential areas.

The safety of the user cannot be guaranteed:

- If the device is operated with accessories that are not supplied or recommended by **IKA®**.
- If the device is operated improperly or in contrary to the **IKA®** specifications.
- If the device or the printed circuit board are modified by third parties.

## Unpacking

- **Unpacking:**


- Please unpack the device carefully.
- In the case of any damage a detailed report must be sent immediately (post, rail or forwarder).

- **Delivery scope:**

- **IKA® MIDI MR 1 digital** or **MAXI MR 1 digital** according to order
- Magnetic stirring bar
- Mains cable
- USB 2.0 cable A – B
- Operating instructions
- Warranty Card.

## Commissioning

Check whether the voltage specified on the type plate matches the mains voltage available.




If above conditions are met, the device is ready for operation after plugging in the mains plug.

If these conditions are not met, safe operation is not guaranteed and the device could be damaged.

Observe the ambient conditions (temperature, humidity, etc.) listed under **“Technical Data”**.

The device can be operated in two modes, **“Continuous mode”** or **“Timer mode”**:

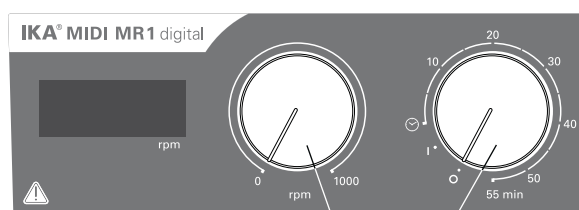

**Fig. 3**

**C**

**B**

- **Continuous mode:**

- ☞ To switch the device on, turn the **“On/Off”** and **“Timer”** rotary knob (**B**, see **Fig. 3**) clockwise to the **“1”** position.
- ⇒ The device is now running in **“Continuous mode”**.
- ☞ To switch the device off, turn the **“On/Off”** and **“Timer”** rotary knob (**B**) to **“0”** position.

- **Timer mode:**

- ☞ To switch the device on, turn the **“On/Off”** and **“Timer”** rotary knob (**B**) clockwise after the **“∞”** position.
- ⇒ The running time can be adjusted to any value between 0 and 55 minutes.
- ⇒ After the selected time period has elapsed, the switch will automatically return to the **“0”** position and the device will remain switched off.
- ⇒ The time period selected can be adjusted at any time.

- **Setting the motor speed:**

- ☞ Set the motor speed by turning the **“Speed”** rotary knob (**C**, see **Fig. 3**). The motor speed can be set to between 0 to 1000 rpm for **MIDI MR 1 digital** and 0 to 600 for **MAXI MR1 digital**.

## Interface and output

The device can be connected to a PC and operated with the laboratory software labworldsoft® through the RS 232 interface (G, see Fig. 2) or USB interface (H, see Fig. 2).

**Note:** Please observe the system requirements as well as the operating instruction and help section of the software.

### **USB interface:**

The Universal Serial Bus (USB) is a serial bus for connecting the device to the PC. Equipped with USB devices can be connected to a PC during operation (hot plugging). Connected devices and their properties are automatically recognized.

Use the USB interface in conjunction with labworldsoft® for operation in "Remote" mode and also to update the firmware.

### **USB device drivers:**

First, download the latest driver for IKA® devices with USB interface from:

<http://www.ika.com/ika/lws/download/usb-driver.zip>.

Install the driver by running the setup file. Then connect the IKA® device through the USB data cable to the PC.

The data communication is via a virtual COM port. Configuration, command syntax and commands of the virtual COM ports are as described in RS 232 interface.

### **RS 232 interface:**

Configuration:

- The functions of the interface connections between the device and the automation system are chosen from the signals specified in EIA standard RS 232 in accordance with DIN 66 020 Part 1.
- For the electrical characteristics of the interface and the allocation of signal status, standard RS 232 applies in accordance with DIN 66 259 Part 1.
- Transmission procedure: asynchronous character transmission in start-stop mode.
- Type of transmission: full duplex.
- Character format: character representation in accordance with data format in DIN 66 022 for start-stop mode. 1 start bit; 7 character bits; 1 parity bit (even); 1 stop bit.

- Transmission speed: 9600 bit/s.
- Data flow control: none.
- Access procedure: data transfer from the device to the computer takes place only at the computer's request.

### **Command syntax and format:**

The following applies to the command set:

- Commands are generally sent from the computer (Master) to the device (Slave).
- The device sends only at the computer's request. Even fault indications cannot be sent spontaneously from the device to the computer (automation system).
- Commands are transmitted in capital letters.
- Commands and parameters including successive parameters are separated by at least one space (Code: hex 0x20).
- Each individual command (incl. parameters and data) and each response are terminated with Blank CR LF (Code: hex 0x20 hex 0x0d hex 0x20 hex 0x0A) and have a maximum length of 80 characters.
- The decimal separator in a number is a dot (Code: hex 0x2E).

The above details correspond as far as possible to the recommendations of the NAMUR working party (NAMUR recommendations for the design of electrical plug connections for analogue and digital signal transmission on individual items of laboratory control equipment, rev. 1.1).

The NAMUR commands and the additional specific IKA® commands serve only as low level commands for communication between the device and the PC. With a suitable terminal or communications programme these commands can be transmitted directly to the device. The IKA® software package, Labworldsoft®, provides a convenient tool for controlling the device and collecting data under MS Windows, and includes graphical entry features, for motor speed ramps for example.

### **Commands:**


Commands	Function
IN_NAME	Input description name.
IN_SP_4	Reading the set rated value of rpm.
IN_PV_4	Reading the real value of rpm.
OUT_SP_4 n	Setting the rated value of rpm to n.
OUT_SP_42@n	Setting the WD safety speed with the echo of the set value
OUT_WD1@m	Watchdog mode 1: When a WD1 event occurs, the stirring functions are shut down and message PC 1 is displayed. Set the watchdog time to m (20...1500) seconds, with echo of the watchdog time. This instruction starts the watchdog function and must be sent within the set watchdog time.

OUT_WD2@m	Watchdog mode 2: When a WD2 event occurs, the speed set point will be set to the WD safety set point speed. The PC 2 warning is displayed. The WD2 event can be reset with OUT_WD2@0-resetting also blocks the watchdog function. Set the watchdog time to m (20...1500) seconds, with echo of the watchdog time. This command starts the watchdog function and must be sent within the set watchdog time.
RESET	Switching off the device function.
START_4	Starting the device (remote) function
STATUS_4	Display of status: 10: Manual operation without fault 11: Automatic operation Start (without fault) 12: Automatic operation Stop (without fault) < 0: error code: - 1: error 1 - ... (see „ <b>Error codes</b> “ table)

**Note:** when disconnecting the RS 232 or USB cable while the device is running, the device stays in PC mode. To reset to function without PC, switch the device off and on again.

**PC 1.1 Cable:**


This cable is required to connect RS 232 interface (G) to a PC.

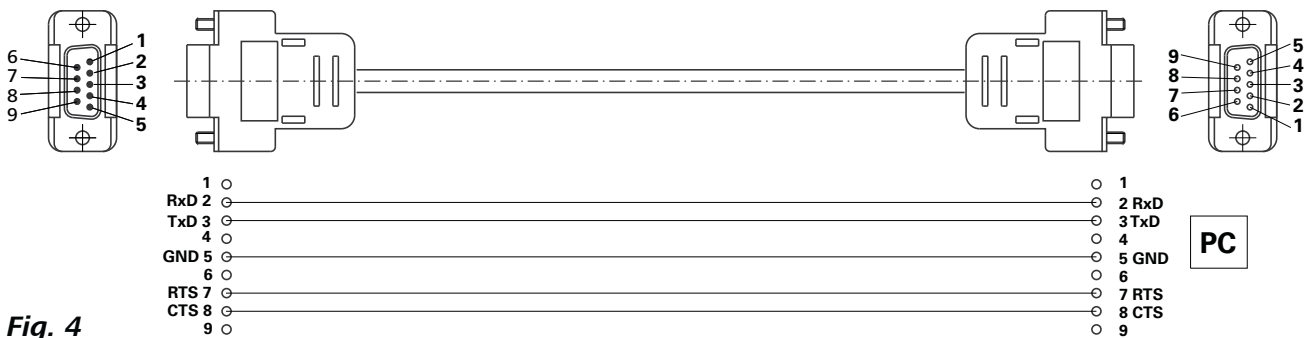

**Fig. 4**

**USB 2.0 cable A - B:**

This cable is required to connect USB interface (H) to a PC.

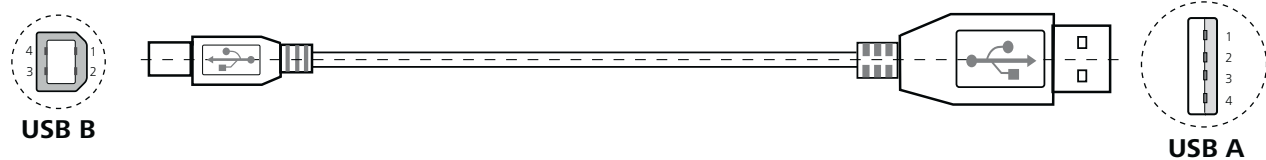


**Fig. 5**

## Maintenance and cleaning

The device is maintenance-free. It is only subject to the natural wear and tear of components and their statistical failure rate.

### Cleaning:



Use only cleaning agents which have been approved by **IKA®** to clean **IKA®** devices.

Dirt	Cleaning agent
Dye	Isopropyl alcohol
Construction material	Water containing tenside/isopropyl alcohol
Cosmetics	Water containing tenside/isopropyl alcohol
Foodstuff	Water containing tenside
Fuel	Water containing tenside

For materials which are not listed, please request information from **IKA®** application support.

Wear protective gloves while cleaning the device.

Electrical devices may not be placed in the cleansing agent for the purpose of cleaning.

Do not allow moisture to get into the device when cleaning.

If a different cleaning or decontamination method than the method defined by **IKA®** is planned, the user must ascertain with **IKA®** that this method does not damage the device.

### Spare parts order:

When ordering spare parts, please give:

- Machine type.
- Serial number, see type plate.
- Item and designation of the spare part, see [www.ika.com](http://www.ika.com), spare parts diagram and list.

### Repair:

**Please send the device for repair only after it has been cleaned and is free from any materials which may constitute a health hazard.**

For repair, please request the “**Decontamination Certificate**” from **IKA®**, or download printout of it from the **IKA®** website [www.ika.com](http://www.ika.com).

Return the device in its original packaging. Storage packaging is not sufficient. Also, please use suitable shipping package materials.

## Error codes

Any malfunctions during operation will be identified by an error message on the display.

Proceed as follows in such cases:

- ☞ Switch off device using the main switch at the back of the device.
- ☞ Carry out corrective measures.
- ☞ Restart device.

Error code	Effect	Cause	Solution
<b>Err 10</b>	Stirring function doesn't start.	Speed setting signal error.	- Contact <b>IKA®</b> service department.
<b>Err 14</b>	Stop stirring or change according to relating setting.	PC communication failure	- Check communication cable.

If the actions described fails to resolve the fault or another error code is displayed then take one of the following steps:

- Contact the service department
- Send the device for repair, including a short description of the fault.

## Accessories

- **IKAFLON®** Magnetic stirring bar
- **TRIKA®** Magnetic stirring bar
- **RSE** Stirring bar remover
- **PC 1.1** Cable
- **Labworldsoft®**

See more accessories on [www.ika.com](http://www.ika.com).

## Technical data

		MIDI MR 1 digital	MAXI MR 1 digital
Operating voltage	<b>VAC</b>	230 ± 10 % 115 ± 10 % 100 ± 10 %	
Frequency	<b>Hz</b>	50 / 60	
Power input	<b>W</b>	70	80
Power output	<b>W</b>	19	35
Max. load on top surface	<b>kg</b>	75	200
Stirred quantity max. (H <sub>2</sub> O)	<b>ltr</b>	50	150
Maximum magnetic bar (L x Ø)	<b>mm</b>	80 x 10	155 x 27
Infinitely adjustable speed range	<b>rpm</b>	0 ... 1000	0 ... 600
Speed tolerance		< ± 10 % of maximum speed	
Speed display		LED	
Operating mode		continuous operation and timer	
Timer	<b>min</b>	∞ / 1 ... 55	
Interface		USB, RS 232	
Fuse	<b>A</b>	2 x T 4 A 250 V	
Permissible ambient temperature	<b>°C</b>	+ 5 ... + 40	
Permitted ambient humidity	<b>%</b>	80	
Permitted on-time	<b>%</b>	100	
Protection class according to EN 60 529		IP 21	
Working plate dimensions (W x D)	<b>mm</b>	350 x 350	500 x 500
Working plate material		stainless steel 1.4301	
Dimensions (W x D x H)	<b>mm</b>	360 x 430 x 110	505 x 585 x 110
Weight	<b>kg</b>	10.7	16
Operation at a terrestrial altitude		max. 2000	

*Subject to technical changes!*

## Warranty

In accordance with **IKA**<sup>®</sup> warranty conditions, the warranty period is 24 months. For claims under the warranty please contact your local dealer. You may also send the machine direct to our factory, enclosing the delivery invoice and giving reasons for the claim. You will be liable for freight costs.

The warranty does not cover worn out parts, nor does it apply to faults resulting from improper use, insufficient care or maintenance not carried out in accordance with the instructions in this operating manual.

[www.imlab.eu](http://www.imlab.eu)

info@imlab.be - Tél. : +32 (0)16 73 55 72

**imLab**

[www.imlab.eu](http://www.imlab.eu)

info@imlab.fr - Tél. : +33 (0)3 20 55 19 11

Imlab sprl - Oude Vijvers, 1  
3370 Boutersem - Belgique

Imlab sarl - Centre d'Affaires de l'Horlogerie  
48 rue des Canoniers - 59000 Lille - France